


# Test report

Number:W202009812E

page1/2

|   |   |   |  |
|---|---|---|--|
| Name of Customer  | Quanzhou City Quanyi Toilet Articles Co.,Ltd  | Address   | No.65 , XiaoWuTang Community, LingYuan Street, JinJiang City, QuanZhou City, FuJian Province |
| Manufacturer  | ---   | Address   | ---  |
| Sample information  | Name of sample: KN95 mask<br>Characteristics of sample: WHITE<br>Trademark of sample: ---<br>Specification/model: ---<br>Level: ---<br>Category of safety specification: ---<br>Art. No. : ---<br>----- |   |  |
| Above-mentioned information by Customer-supplied            |   |   |  |
| The sent way of sample                                      | Courier   | Sample quantity   | 30 pieces  |
| Receiving Date of Sample                                    | 2020/04/23  | Test Category   | Entrusted inspection   |
| Date of Testing   | 2020-04-24- 2020-04-28  |   |  |
| RatingRequirements  | GB 2626-2006  |   |  |
| Test Summary:<br><br>See the attached page for the results. |   |   |  |
|   |   | <br>Test Seal<br>Date of Approval: 2020-04-29 |  |
| Remarks   | The sample is not pretreated and the result is for reference.   |   |  |

Approved by:

俞 杰




# Test report

Number:W202009812E

page2/2

| ITEM   | STANDARD<br>(KN95)                                | RESULT   | RATING |
|--|---|--|--------|
| 1. FILTER EFFICIENCY(SALT MEDIUM)<br>(GB 2626-2006 6.3)(%) |   |  |        |
| -  | $\geq 95.0$                                       | 98.1   | PASS   |
| 2. RESPIRATORY RESISTANCE<br>(GB 2626-2006 6.5 & 6.6)(Pa)  |   |  |        |
| -INSPIRATORY RESISTANCE                                    | $\leq 350$  | 115  | PASS   |
| -EXPIRATORY RESISTANCE                                     | $\leq 250$  | 101  | PASS   |
| 3. HEADBAND<br>(GB 2626-2006 6.11)                         |   |  |        |
| -  | $\geq 10N$ ,hold on10s                            | No breakage and<br>slippage were observed                        | PASS   |
| 4. APPEARANCE<br>(GB 2626-2006 6.1 & 6.2)                  |   |  |        |
| -  | Meet the requirements of<br>GB 2626-2006 standard | The appearance quality<br>of 2 masks conforms to<br>the standard | PASS   |
| 5.VISUAL FIELD BELOW MASK<br>(GB 2890-2009)(° )            |   |  |        |
| -  | $\geq 60$   | 75   | PASS   |

Picture(s) of sample

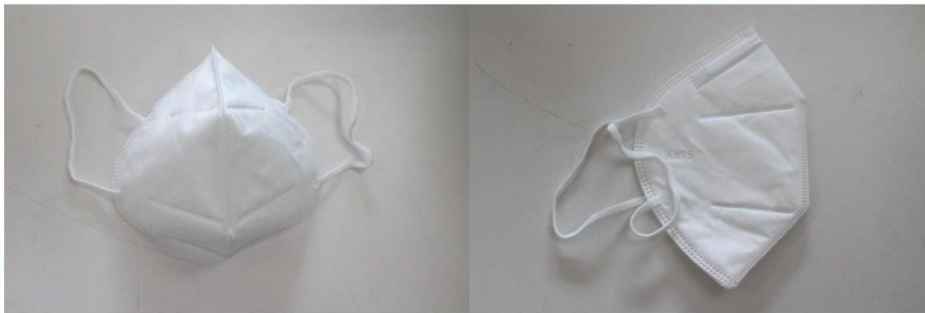

—End of report—

